

Current Data Parameters
 NAME B2
 EXPNO 21
 PROCNO 1


F2 - Acquisition Parameters

INSTRUM spect
 PROBHD 5 mm CPQCI 1H/
 PULPROG zg30
 TD 65536
 SOLVENT DMSO
 NS 1
 DS 0
 SWH 10000.000 Hz
 FIDRES 0.152588 Hz
 AQ 3.2767999 sec
 RG 21.83
 DW 50.000 usec
 DE 10.00 usec
 TE 296.1 K
 D1 1.00000000 sec
 TD0 1

==== CHANNEL f1 =====
 SFO1 500.1530886 MHz
 NUC1 1H
 P1 10.80 usec
 PLW1 4.37519979 W

F2 - Processing parameters
 SI 65536
 SF 500.1500100 MHz
 WDW EM
 SSB 0
 LB 0.10 Hz
 GB 0
 PC 1.00

成都普菲德生物技术有限公司
 www.sc-victory.com

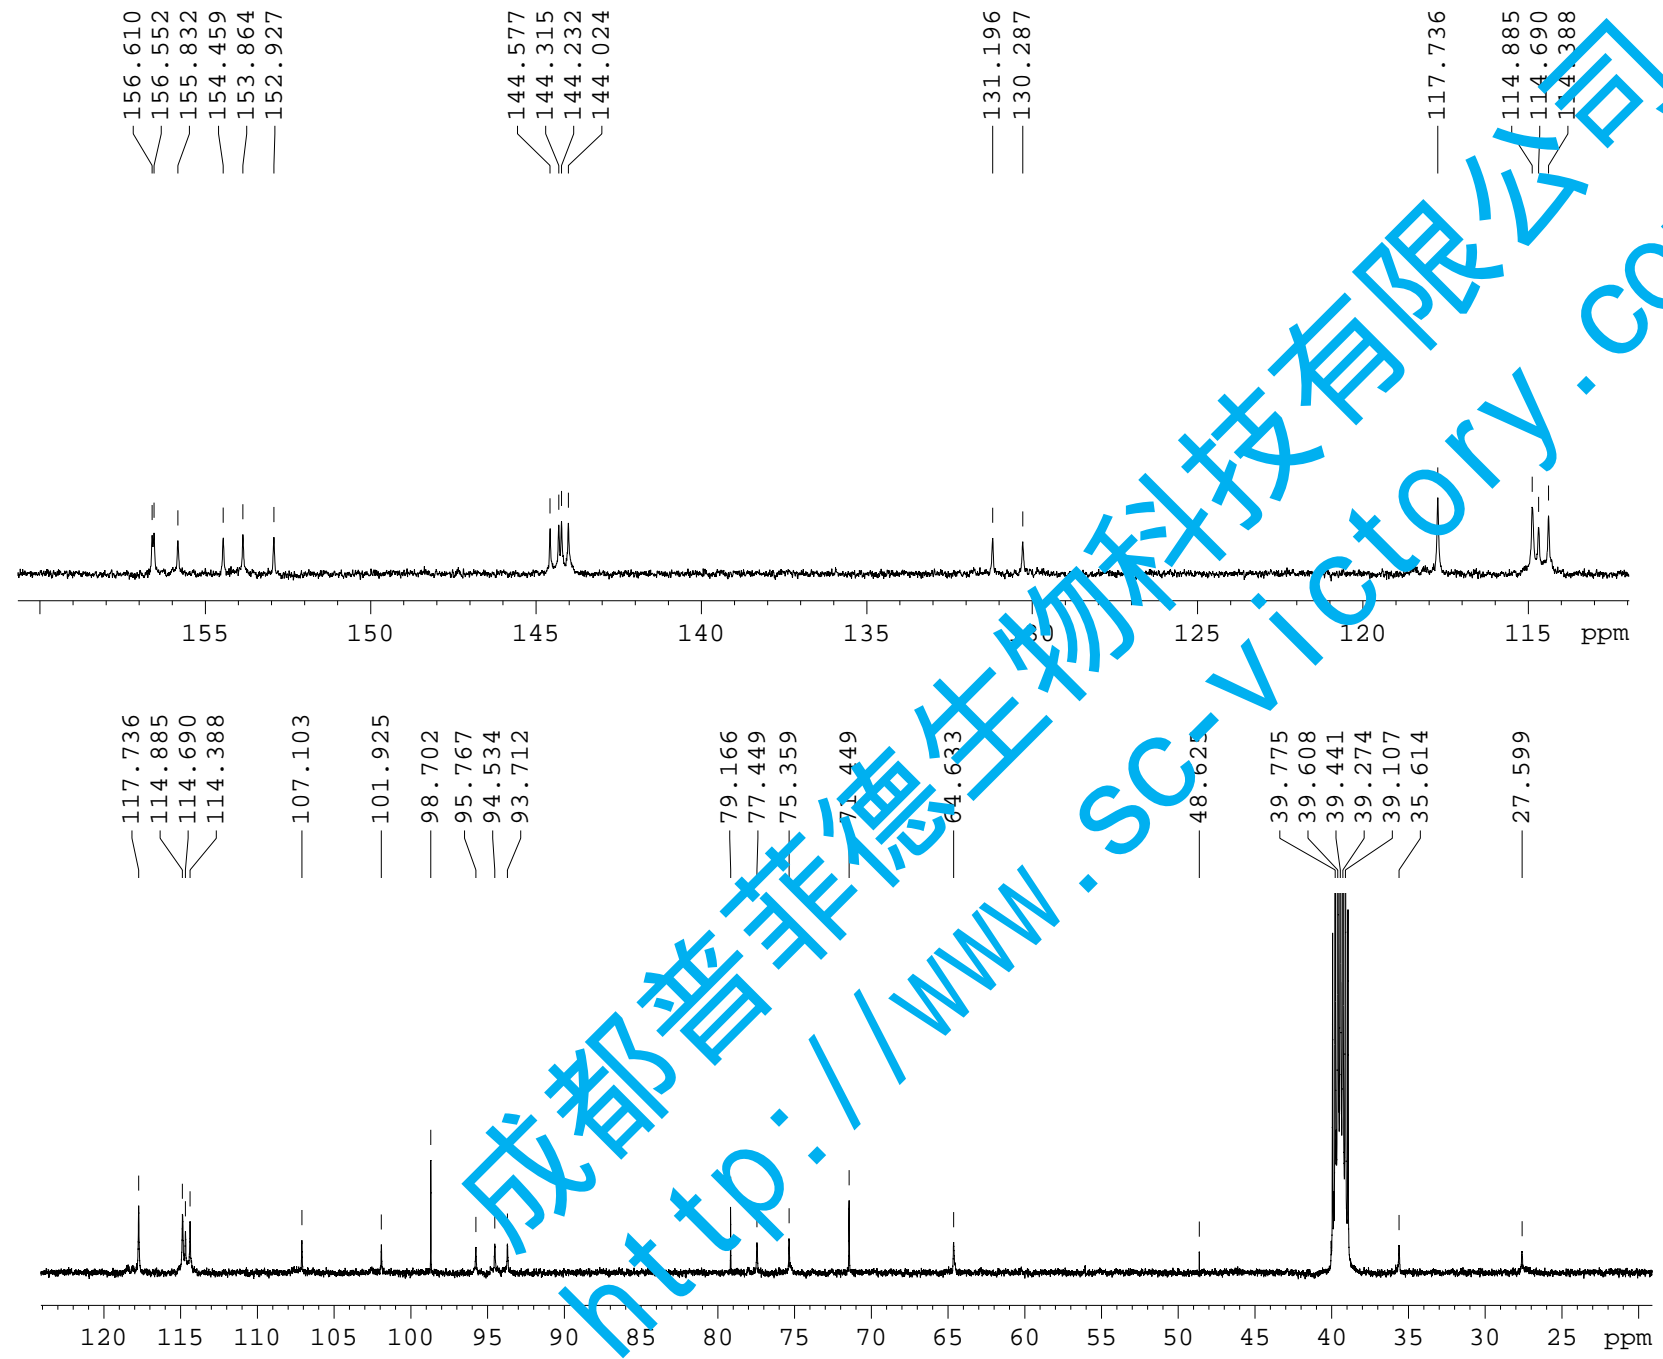

```

Current Data Parameters
=====
v.ME      B2
EXPNO     42
PROCNO    1

F2 - Acquisition Parameters
=====
INSTRUM   spect
PROBHD    5 mm CPQCI 1H/
PULPROG   zgdc
TD        65536
SOLVENT   DMSO
NS        512
DS        4
SWH       29761.904 Hz
FIDRES    0.454131 Hz
AQ        1.1010048 sec
RG        187.72
DW        16.800 usec
DE        18.00 usec
TE        296.2 K
D1        3.00000000 sec
D11       0.03000000 sec
TD0       1

===== CHANNEL f1 =====
SFO1      125.7769030 MHz
NUC1      13C
P1        11.70 usec
PLW1      160.00000000 W

===== CHANNEL f2 =====
SFO2      500.1527508 MHz
NUC2      1H
CPDPRG[2] waltz16
PCPD2     100.00 usec
PLW2      4.37519979 W
PLW12     0.05390700 W

F2 - Processing parameters
SI        32768
SF        125.7628735 MHz
WDW       EM
SSB       0
LB        1.00 Hz
GB        0
PC        1.40

```